

# IESNA LM-79: 2008

## Measurement and Test Report

for

### Green Creative Ltd.

Room 1206-7, New Victory House, 93-103 Wing Lok Street, Central, HONG KONG

Sep 29, 2013

<b>Product Name:</b>	LED PAR30SN
<b>Model No:</b>	14.5PAR30SNG3DIM/830FL40
<b>Test Engineer:</b>	David Zhang 
<b>Report No.:</b>	BTR66.181.13.1428.01
<b>Sample Received Date:</b>	Sep 26, 2013
<b>Test Performed Date:</b>	Sep 26, 2013 to Sep 29, 2013
<b>Reviewed By:</b>	Steven Hsu 
<b>Prepared By:</b>	<b>BEST Test Service Shenzhen Co., Ltd.</b> 1st Floor, 1st Building, Weitai Industrial Park, Yingrenshi, Shiyan, Baoan, Shenzhen, China TEL: +86-755-28236006 FAX: +86-755-23467087-811 Email: <a href="mailto:certification@bestcert.cn">certification@bestcert.cn</a>



**Note:** The test report only allows to be revised within the retention period unless further standard or the requirement was noticed. This report is for the exclusive use of BEST's Client and is provided pursuant to the agreement between BEST and its Client. BEST's responsibility and Liability are limited to the terms and conditions of the agreement. BEST assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the BEST name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by BEST. The observations and test results in this report are relevant only to the sample tested. This report by itself does not cover that the material, product, of service is or has ever been under a BEST certification program. National Voluntary Laboratory Accreditation Program (NVLAP) has accredited this laboratory under ISO17025: 2005 for specific laboratory activities as listed in the NVLAP directory of accredited laboratories. The results shown in this report were determined by this laboratory in accordance with its terms of accreditation.

**TABLE OF CONTENTS**

**1 - GENERAL INFORMATION.....3**

- 1.1 PRODUCT DESCRIPTION FOR EQUIPMENT UNDER TEST (EUT) .....3
- 1.2 OBJECTIVE .....3
- 1.3 TEST FACILITY DESCRIPTION.....4
- 1.4 TEST EQUIPMENT LIST .....4

**2 - TEST METHOD.....5**

- 2.1 PHOTOMETRIC AND ELECTRICAL MEASUREMENT (INTEGRATED SPHERE METHOD) .....5
- 2.2 PHOTOMETRIC AND ELECTRICAL MEASUREMENT (GONIOPHOTOMETER METHOD) .....5
- 2.3 DEVIATION FROM STANDARD OPERATING PROCEDURE .....5

**3 – SUMMARY OF TEST RESULT .....6**

**4 – SPECTRAL FLUX PLOTS .....8**

**5 – EUT PHOTOS.....9**

**6 – LUMINOUS INTENSITY DISTRIBUTION TEST PLOTS (CIE CHROMATICITY).....10**



## 1 - GENERAL INFORMATION

### 1.1 Product Description for Equipment under Test (EUT)

Applicant	:	Green Creative Ltd.
Product Name	:	LED PAR30SN
Model No	:	14.5PAR30SNG3DIM/830FL40
Brand	:	GREEN CREATIVE
SKU	:	T.B.D
12 NC Code	:	T.B.D
Nominal Operation Voltage	:	AC 120V/60Hz
Nominal Power	:	14.5W
Nominal CCT	:	3000K
Nominal CRI	:	82
Nominal Lumen Output	:	850Lumens
Nominal Life Time	:	40000Hours
Number of hours operated prior to measurement for new sample	:	0 Hours
Stabilization Time	:	1.5 hours
Total operating time for measurement include stabilization time	:	3.5 hours
		<input checked="" type="checkbox"/> Standard <input type="checkbox"/> Non Standard
Nominal Shape of Bulb(Designation)	:	<input type="checkbox"/> Omnidirectional A, BT, P, PS, S, T <input type="checkbox"/> Decorative B, BA, C, CA, DC, F, G <input checked="" type="checkbox"/> Directional R, BR, ER, PAR, MR, K
Date of Receiving Sample	:	Sep 26, 2013
Measurement quantities measured	:	1 pcs
Orientation During Testing	:	Base Up
Test Requested	:	Electrical and Photometric Test Luminous Intensity Distribution Test

### 1.2 Objective

The following test report is prepared on behalf of Green Creative Ltd. in accordance with IESNA LM-79-08, used the following American National Standards or illumination Engineering Society of North America test guides:

- ANSI C78.377-2008: Specifications for the Chromaticity of Solid State Lighting Products;
- ANSI C79.1– 2002: American National Standard for Electric Lamps – Nomenclature for Glass Bulbs Intended for Use with Electric Lamps;
- ANSI C78.20 – 2003: American National Standard for Electric Lamps – A, G, PS, and Similar Shapes with E26 Medium Screw Bases;
- ANSI C78.21 – 2011: American National Standard for Electric Lamps – PAR and R Shapes;
- ANSI C78.24 – 2001: American National Standard for Electric Lamps – Two-inch (51 mm); Integral-reflector Lamps with Front Covers and GU5.3 or GX 5.3 Bases;
- ANSI/IEC C81.61-2003: American National Standard for Electric Lamp Bases;
- ANSI/IEEE C62.41 – 1991 (01-May-1991): Surge Voltages in Low-Voltage AC Power Circuits, Recommended Practice for;
- CIE Publication No. 13.3 – 1995: Method of Measuring and Specifying Color Rendering of Light Sources;
- CIE Publication No. 18.2 – 1983: The Basis of Physical Photometry;
- IESNA LM-16-1993: Practical Guide to Colorimetry of Light Sources;
- IESNA LM-28-89 – 1989: Guide for the Selection, Care, and Use of Electrical Instruments in the Photometric Laboratory;
- IESNA LM-79-08 Electrical and Photometric Measurement of Solid State Lighting Products
- UL 1993 – 1999: Standard for Self-Ballasted Lamps and Lamp Adapters;
- UL 8750 – 2009: Light Emitting Diode (LED) Equipment for Use in Lighting Products.

### 1.3 Test Facility Description

The Energy Efficiency Lab used by BEST to collect energy efficiency measurement data is located in 1st Floor, 1st Building, Weitai Industrial Park, Yingrenshi, Shiyao, Baoan, Shenzhen, China. BEST Test Service Shenzhen Co., Ltd is a National Institute of Standards and Technology (NIST) accredited laboratory, under the National Voluntary Laboratory Accredited Program (Lab Code 200770-0). BEST Test Service Shenzhen Co., Ltd is also an ELI accredited lab for lighting products (ELI Certificate No. ELI-L04-2010) and UL accredited lab for lighting products

### 1.4 Test Equipment List

Apparatus List	Device	Cal. Date	Cal Due Date
1	Integral Sphere+ Spectrophotometer System	Mar 10, 2013	Mar 09, 2014
2	Digital Power Meter	Oct 18, 2012	Oct 17, 2013
3	Goniophotometer+ Spectrophotometer System	Nov 20, 2012	Nov 19, 2013
4	Standard Light Source	Sep 17, 2013	Sep 16, 2014
5	Standard Light Source	Sep 17, 2013	Sep 16, 2014
6	Digital Storage Oscilloscope	Oct 18, 2012	Oct 17, 2013
7	Ultra Compact Simulator	Oct 20, 2012	Oct 20, 2013
8	Temperature Chamber	Oct 20, 2012	Oct 20, 2013
9	Digital Caliper	Nov 20, 2012	Nov 19, 2013
10	Digital CC&CV DC Power Supply(30V 5A)	N/A	N/A
11	5 1/2 Digital Multimeter	Oct 18, 2012	Oct 17, 2013
12	Digital CC&CV DC Power Supply(120V 10A)	N/A	N/A
13	6 1/2 Digital Multimeter	Oct 18, 2012	Oct 17, 2013
14	Digital Multimeter	Oct 18, 2012	Oct 17, 2013
15	Temperature Recorder+Thermocouple	Nov 20, 2012	Nov 19, 2013
16	Timer Controller	Nov 20, 2012	Nov 19, 2013

**Statement of Traceability:** BEST Test Service Shenzhen Co., Ltd. certifies that all calibration has been performed using suitable standards traceable to the NIM China.

## 2 - Test Method

---

### 2.1 Photometric and Electrical Measurement (Integrated Sphere Method)

Total light output (luminous flux) for the  $25^{\circ}\text{C} \pm 1^{\circ}\text{C}$  ambient temperature conditions is measured using a 1.6m 4Π geometry integrating sphere. Temperature is measured at a position inside the sphere. Spectral radiant flux measurements are made using Lab sphere to the detector port of the integrating sphere. Each lamp is operated at rated voltage in its designated orientation. Each lamp should be stable before measurements are made. The determining method of stable is as follows:

Step 1 Take 3 measurements of the lamp light output at 15 minute interval (total time=30mintues.)This time period is in addition to the recommended pre-burning time.

Step 2 Calculate the percent difference between the maximum measured value and the minimum measured value for the three consecutive measurements.

Step 3 if the value calculated in Step 2 does not exceed 0.5 percent, the lamp is considered stable. Luminous flux, chromaticity coordinates, correlated color temperature and color rendering index for each lamp are calculated from the spectral radiant flux measurements taken at 2 nm intervals over the range 350 to 1050 nm. The calibration of the sphere photometer-spectrometer system is traceable to the NIST USA. Lamp efficacy (lumens per watts) for each lamp model is computed based on the revised luminous flux result. Electrical measurements including voltage, current, power and power factor are measured using the digital power Meter.

The total uncertainty of the light output measurements is estimated, at the 95% confidence level, not to exceed  $\pm 1.12\%$  over the wavelength range 350-1050 nm.

### 2.2 Photometric and Electrical Measurement (GonioPhotometer Method)

A Goniometer was used to measure the intensity (candelas) at each angle of distribution for each sample; the photometric distance is 24m. Ambient temperature was measured equal to the height of the sample mounted on the Goniometer equipment. Each sample was operated at input rated voltage in its designated orientation. Each sample was allowed to be stable before measurement was made. Electrical measurements including voltage, current, power and power factor were measured using the Power Analyzer

Before each measurement, the method below should be used to determine the lamp is stable or not.

Step 1 Take 3 measurements of the lamp intensity at 15 minute interval (total time=30mintues.)This time period is in addition to the recommended pre-burning time.

Step 2 Calculate the percent difference between the maximum measured value and the minimum measured value for the three consecutive measurements.

Step 3 if the value calculated in Step 2 does not exceed 0.5 percent, the lamp is considered stable.

Some graphics were created with Photometric Plus software.

### 2.3 Deviation from standard operating procedure

None.

### 3 – Summary of Test Result



	Item	Test Result		Accreditation
Required Fields	Lumen Output (Lumens)	917.30		NVLAP/EPA
	Luminous Efficacy (lm/w)	62.67		NVLAP/EPA
	Correlated Color Temperature (CCT)	2999		NVLAP/EPA
	Color Rendering Index– CRI	83.6		NVLAP/EPA
	Input Power (W)	14.64		NVLAP/EPA
Optional Fields	Power Type	<input checked="" type="checkbox"/> AC	<input type="checkbox"/> DC	/
	Input Voltage (V)	120.0		NVLAP/EPA
	Input Current (A)	0.1282		NVLAP/EPA
	Power Factor	0.9509		NVLAP/EPA
	x(CIE 1931)	0.4398		NVLAP/EPA
	y(CIE 1931)	0.4098		NVLAP/EPA
	u' (CIE 1976)	0.2500		NVLAP/EPA
	v' (CIE 1976)	0.5240		NVLAP/EPA
	Duv(CIE 1976)	0.0019		NVLAP/EPA
	Beam Angle: (Degree)	38.3		NVLAP/EPA
	Center beam candlepower: (cd)	1376		NVLAP/EPA
	Zonal lumen density (0-60°):	93.0%		NVLAP/EPA
	Zonal lumen density (60-90°):	7.0%		NVLAP/EPA
	Zonal lumen density (90-120°):	0%		NVLAP/EPA
Zonal lumen density (120-180°):	0%		NVLAP/EPA	

	CRI (R1)	82	NVLAP/EPA
	CRI (R2)	92	NVLAP/EPA
	CRI (R3)	96	NVLAP/EPA
	CRI (R4)	83	NVLAP/EPA
	CRI (R5)	83	NVLAP/EPA
	CRI (R6)	91	NVLAP/EPA
	CRI (R7)	83	NVLAP/EPA
	CRI (R8)	59	NVLAP/EPA
	CRI (R9)	6	NVLAP/EPA
	CRI (R10)	82	NVLAP/EPA
	CRI (R11)	84	NVLAP/EPA
	CRI (R12)	72	NVLAP/EPA
	CRI (R13)	85	NVLAP/EPA
	CRI (R14)	99	NVLAP/EPA

**Lumen summary:**

[OTHER]	Gamma(deg)	Fz(lm)	Ft(lm)	%Lum	%Lamp
[OTHER]	0- 10	118.40	118.40	12.91	12.91
[OTHER]	10- 20	242.62	361.02	39.36	39.36
[OTHER]	20- 30	214.31	575.34	62.72	62.72
[OTHER]	30- 40	142.05	717.39	78.21	78.21
[OTHER]	40- 50	84.63	802.02	87.43	87.43
[OTHER]	50- 60	51.12	853.14	93.01	93.01
[OTHER]	60- 70	35.15	888.29	96.84	96.84
[OTHER]	70- 80	22.09	910.37	99.25	99.25
[OTHER]	80- 90	6.88	917.26	100.00	100.00
[OTHER]	90-100	0.04	917.30	100.00	100.00
[OTHER]	100-110	0.00	917.30	100.00	100.00
[OTHER]	110-120	0.00	917.30	100.00	100.00
[OTHER]	120-130	0.00	917.30	100.00	100.00
[OTHER]	130-140	0.00	917.30	100.00	100.00
[OTHER]	140-150	0.00	917.30	100.00	100.00
[OTHER]	150-160	0.00	917.30	100.00	100.00
[OTHER]	160-170	0.00	917.30	100.00	100.00
[OTHER]	170-180	0.00	917.30	100.00	100.00

## 4 – Spectral Flux Plots

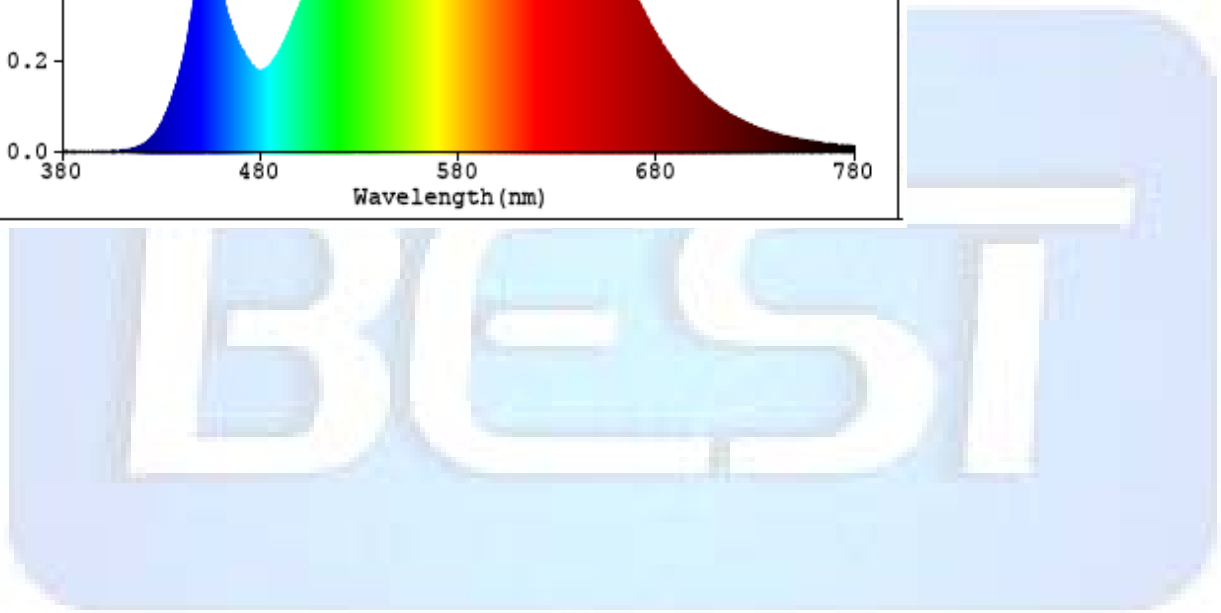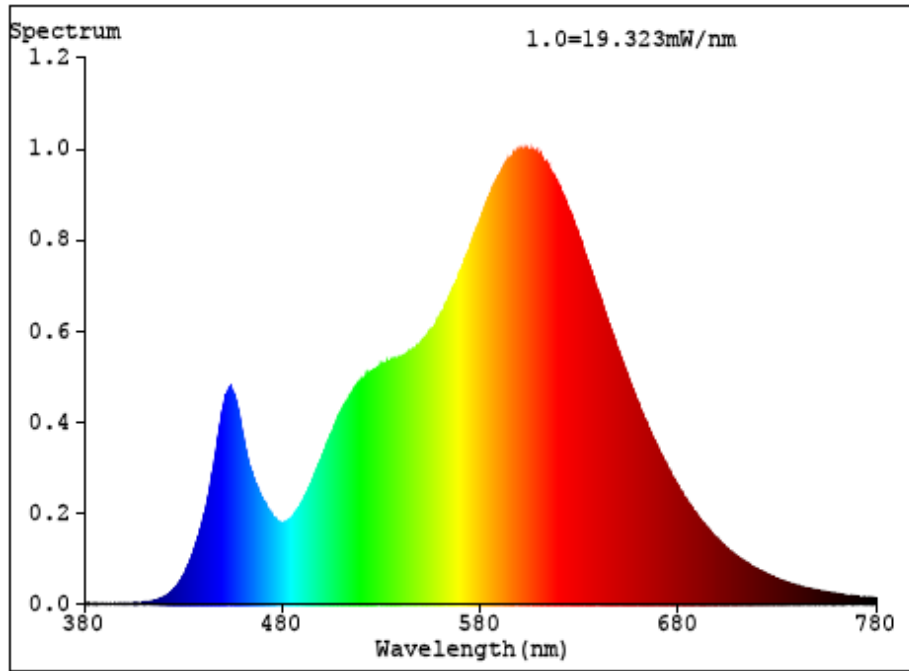




## 5 – EUT Photos



## 6 – Luminous Intensity Distribution Test Plots (CIE Chromaticity)

### LAMP PHOTOMETRIC REPORT

Electrical: Voltage:120.0V Current:0.1282A Power:14.64W Factor:0.9509		
MODEL: 14.5PAR30SNG3DIM/830FL40		
POWER: 14.5W	VOLTAGE: 120V	WORKING VOLTAGE: 120.0V
MANUFACTURER: Green Creative		Eff.: 62.67 lm/W

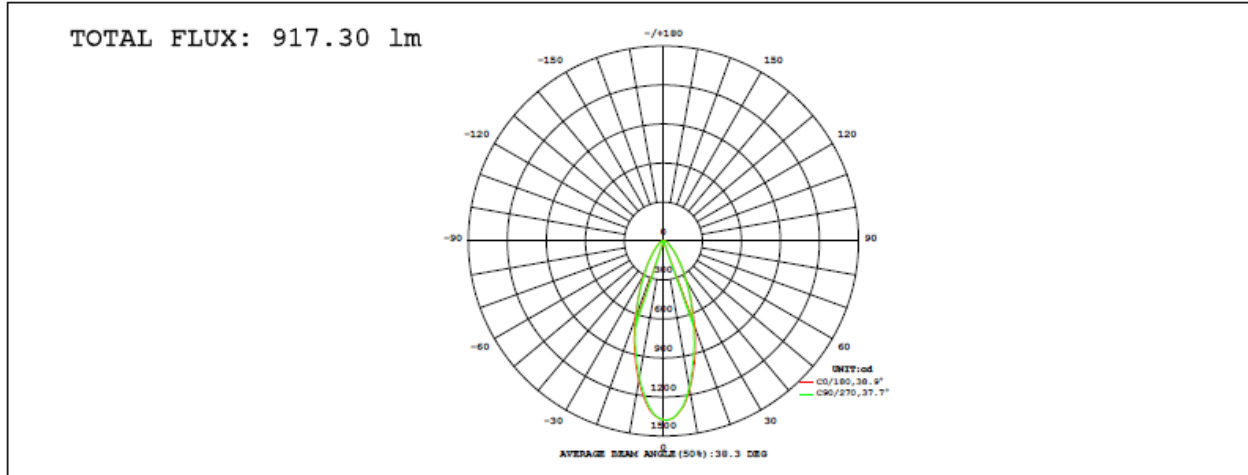

γ	C0	C45	C90	C135	C180	C225	C270	C315	γ	Φ zone	Φ total	%
10	1092	1059	1065	1111	1159	1152	1142	1132	0- 10	118.4	118.4	12.9
20	637.8	603.5	612.0	653.7	699.9	686.3	669.8	666.8	10- 20	242.6	361.0	39.4
30	307.1	290.3	293.8	314.4	349.2	356.0	347.1	332.6	20- 30	214.3	575.3	62.7
40	143.6	133.3	133.9	144.1	166.2	175.8	173.1	160.4	30- 40	142.0	717.4	78.2
50	70.29	66.28	66.23	70.74	80.66	87.69	86.73	78.82	40- 50	84.63	802.0	87.4
60	41.87	39.81	39.72	42.08	45.51	48.30	48.10	45.05	50- 60	51.12	853.1	93
70	26.93	25.49	25.49	26.93	29.10	30.85	30.70	29.10	60- 70	35.15	888.3	96.8
80	12.05	10.93	11.17	12.36	14.80	16.17	16.06	14.51	70- 80	22.09	910.4	99.2
90	0.0011	0	0	0.0075	0.5623	1.575	1.361	0.2905	80- 90	6.885	917.3	100
100	0	0	0	0	0	0	0	0	90-100	0.0366	917.3	100
110	0	0	0	0	0	0	0	0	100-110	0	917.3	100
120	0	0	0	0	0	0	0	0	110-120	0.0000	917.3	100
130	0	0	0	0	0	0	0	0	120-130	0	917.3	100
140	0	0	0	0	0	0	0	0	130-140	0	917.3	100
150	0	0	0	0	0	0	0	0	140-150	0	917.3	100
160	0	0.0000	0	0	0.0002	0.0007	0.0002	0.0012	150-160	0.0000	917.3	100
170	0.0078	0.0090	0.0085	0.0083	0.0088	0.0076	0.0079	0.0092	160-170	0.0011	917.3	100
180	0	0	0	0	0	0	0	0	170-180	0.0006	917.3	100
DEG	LUMINOUS INTENSITY:cd								UNIT:lm			

C Range: 0 - 360DEG  
 C Interval: 22.5DEG  
 Test Speed: HIGH  
 Temperature:25.2DEG  
 Operators:David

γ Range: 0 - 180DEG  
 γ Interval: 1.0DEG  
 Test System:EVERFINE GO-R5000\_V2 SYSTEM V2.0.265  
 Humidity:62.7%  
 Test Distance:2.456m [K=1.0000]

LUMINOUS DISTRIBUTION INTENSITY DATA

Electrical: Voltage:120.0V Current:0.1282A Power:14.64W Factor:0.9509		
MODEL: 14.5PAR30SNG3DIM/830FL40		
POWER: 14.5W	VOLTAGE: 120V	WORKING VOLTAGE: 120.0V
MANUFACTURER: Green Creative		Eff.: 62.67 lm/W

Table--1

UNIT: cd

C (DEG) \ y (DEG)	0	23	45	68	90	113	135	158	180	203	225	248	270	293	315	338			
0	1376	1375	1375	1374	1374	1374	1374	1373	1376	1375	1375	1374	1374	1374	1374	1373			
5	1293	1280	1272	1270	1276	1287	1302	1316	1327	1330	1329	1327	1323	1318	1314	1310			
10	1092	1072	1059	1055	1065	1086	1111	1131	1159	1158	1152	1145	1142	1137	1132	1122			
15	859	838	824	822	832	855	884	908	932	925	913	902	898	897	898	891			
20	638	616	603	603	612	630	654	676	700	695	686	677	670	668	667	659			
25	446	432	424	423	430	443	461	480	502	502	498	493	485	480	475	467			
30	307	297	290	290	294	301	314	330	349	354	356	354	347	340	333	324			
35	213	204	198	197	200	205	214	226	244	251	254	255	249	242	234	226			
40	144	137	133	133	134	137	144	153	166	172	176	177	173	167	160	154			
45	100	95.9	93.1	92.2	93.1	95.6	100	106	116	121	125	127	124	119	113	108			
50	70.3	67.8	66.3	65.6	66.2	68.0	70.7	74.5	80.7	84.4	87.7	88.9	86.7	83.0	78.8	75.1			
55	52.5	51.1	50.1	49.5	50.0	51.3	53.0	55.2	58.5	60.9	63.0	63.7	62.5	60.1	57.6	55.4			
60	41.9	40.7	39.8	39.2	39.7	40.8	42.1	43.6	45.5	47.1	48.3	48.6	48.1	46.7	45.1	43.9			
65	34.0	33.0	32.2	31.5	32.1	33.0	34.0	35.1	36.6	37.9	38.7	38.7	38.5	37.6	36.4	35.6			
70	26.9	26.1	25.5	25.0	25.5	26.1	26.9	27.8	29.1	30.2	30.8	30.8	30.7	30.0	29.1	28.4			
75	19.8	18.9	18.5	18.2	18.7	19.0	19.9	20.8	22.2	23.1	23.6	23.7	23.6	22.9	22.1	21.3			
80	12.1	11.3	10.9	10.8	11.2	11.6	12.4	13.3	14.8	15.7	16.2	16.4	16.1	15.3	14.5	13.5			
85	4.87	4.22	3.89	3.83	4.10	4.57	5.21	5.97	7.26	7.96	8.38	8.56	8.19	7.64	6.90	6.01			
90	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.03	0.56	1.24	1.58	1.63	1.36	0.93	0.29	0.00			
95	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
100	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
105	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
110	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
115	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
120	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
125	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
130	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
135	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
140	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
145	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
150	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
155	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
160	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			
165	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.01		
170	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01		
175	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00		
180	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00			

C Range: 0 - 360DEG  
 C Interval: 22.5DEG  
 Test Speed: HIGH  
 Temperature:25.2DEG  
 Operators:David

y Range: 0 - 180DEG  
 y Interval: 1.0DEG  
 Test System:EVERFINE GO-R5000\_V2 SYSTEM V2.0.265  
 Humidity:62.7%  
 Test Distance:2.456m [K=1.0000]